

Analytical Test Result


CaptureSelect™
AAVX Ligand Leakage ELISA
Origin: The Netherlands

Catalogue Code: 810352201
810352210
Lot Number: 010721-107
Expiration Date: Jan 2027
Manufacturing Date: Jan 2023
Storage Temperature: -30/-5 °C

Content of the kit:

Reagents	Description	Lot number	Concentration (OD _{280nm})
Coating reagent	Goat IgG anti-AAVX affinity ligand	210620	0.14 mg/ml
Standard solution	CaptureSelect AAVX affinity ligand	210621	0.5 mg/ml
Biotinylated reagent	Biotinylated Goat IgG anti-AAVX affinity ligand	210622	0.16 mg/ml

MATERIAL REF. & TEST	SPECIFICATION	Test RESULT	UNITS
Internal control recover (Reference standard 4.2 ng/ml)	80 – 120	107 4.2	% ng/mL
Sensitivity (Ligand detection limit)	≤ 1	Conform	ng/mL
Calibration curve (ELISA)	Conform	See below	
TMB incubation time (BD OptEIA TMB)	2-20	5	minutes

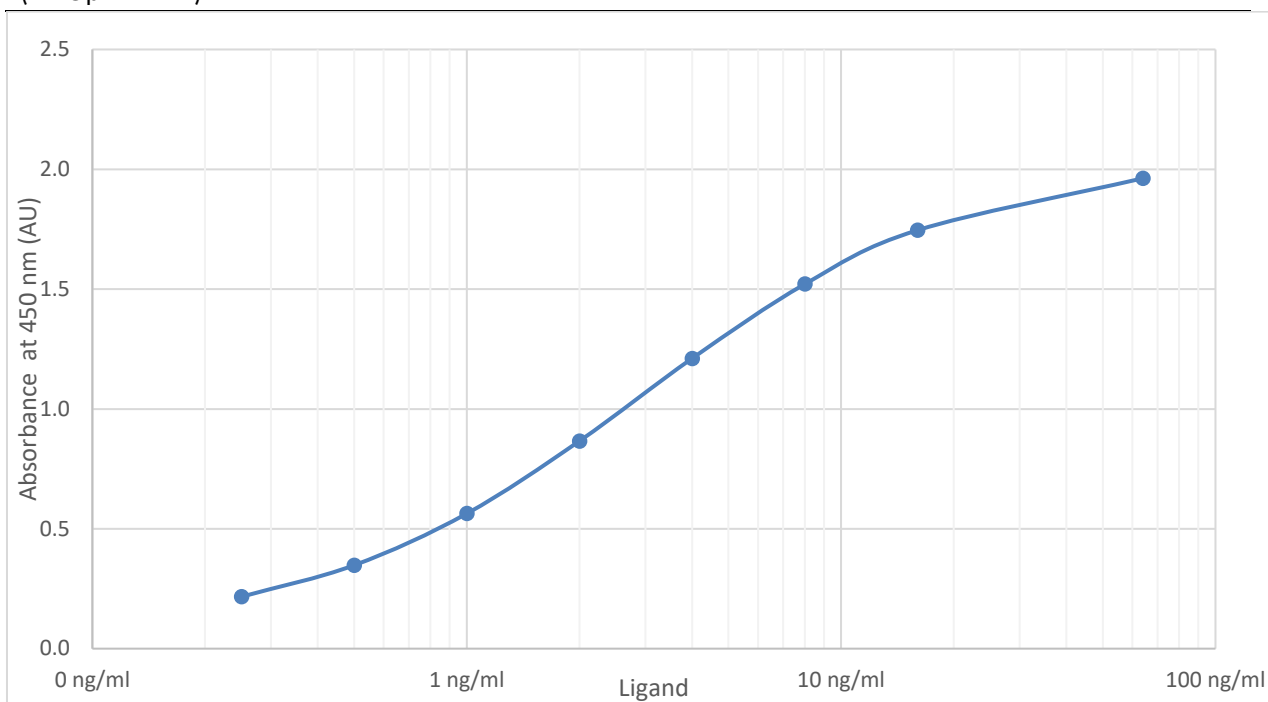

Example of calibration curve, Lot 010721-107 (y-axis OD_{450nm}; x-axis [Ligand] in ng/mL)
FOR RESEARCH ONLY. NOT INTENDED FOR HUMAN USE

Product management

Date: 2-Jun-2023