

## Analytical Test Result


**CaptureSelect™**  
**AAVX Ligand Leakage ELISA**  
Origin: The Netherlands

Catalogue Code: 810352201  
810352210  
Lot Number: 010721-108  
Expiration Date: Apr 2027  
Manufacturing Date: Apr 2023  
Storage Temperature: -30/-5 °C

### Content of the kit:

Reagents	Description	Lot number	Concentration (OD <sub>280nm</sub> )
Coating reagent	Goat IgG anti-AAVX affinity ligand	210620	0.14 mg/ml
Standard solution	CaptureSelect AAVX affinity ligand	210621	0.5 mg/ml
Biotinylated reagent	Biotinylated Goat IgG anti-AAVX affinity ligand	210622	0.16 mg/ml

MATERIAL REF. & TEST	SPECIFICATION	Test RESULT	UNITS
<b>Internal control recover</b> (Reference standard 4.2 ng/ml)	80 – 120	105 4.2	% ng/mL
<b>Sensitivity</b> (Ligand detection limit)	≤ 1	Conform	ng/mL
<b>Calibration curve</b> (ELISA)	Conform	See below	
<b>TMB incubation time</b> (BD Opteia TMB)	2-20	6.5	minutes

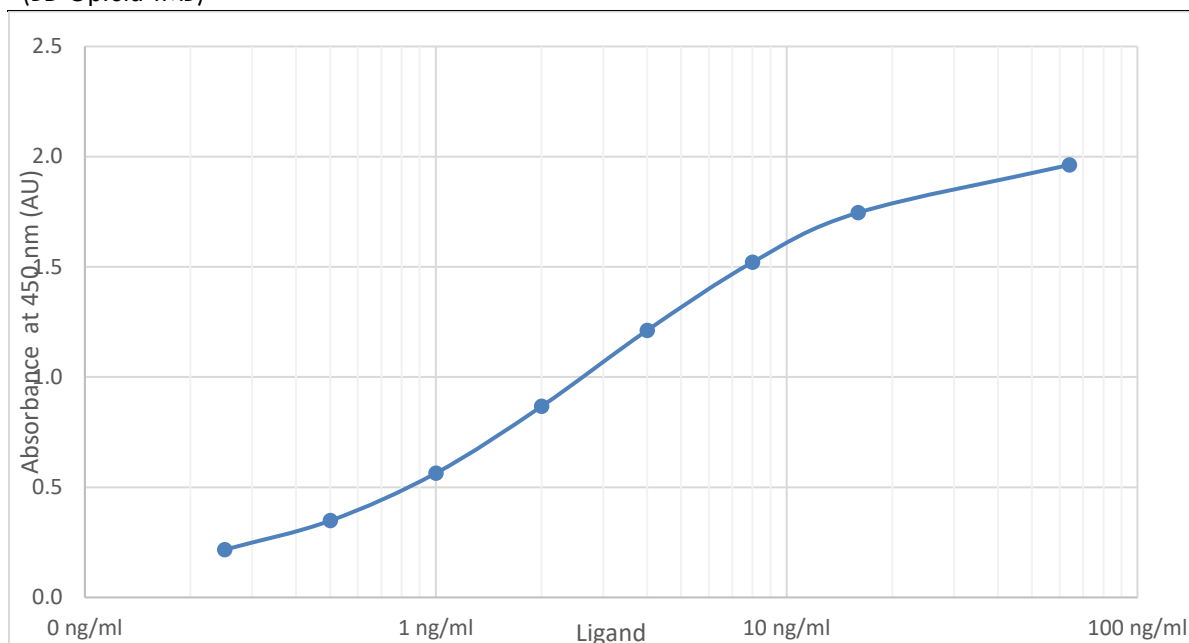

Example of calibration curve, Lot 010721-108 (y-axis OD<sub>450nm</sub>; x-axis [Ligand] in ng/mL)  
**FOR RESEARCH ONLY. NOT INTENDED FOR HUMAN USE**

Product management

Date: 2-Jun-2023