

Analytical Test Result

CaptureSelect™
AAVX Ligand Leakage ELISA
Origin: The Netherlands


Catalogue Code: 8103522xx
Lot Number: 101017-211

Expiration Date: Jun 2026
Manufacturing Date: Jun 2022
Storage Temperature: -25-/15 °C

Content of the kit:

Reagents	Description	Lot number	Concentration (OD _{280nm})
Coating reagent	Goat IgG anti-AAVX affinity ligand	170908	0.26 mg/ml
Standard solution	CaptureSelect AAVX affinity ligand	170910	0.5 mg/ml
Biotinylated reagent	Biotinylated Goat IgG anti-AAVX affinity ligand	170909	0.27 mg/ml

MATERIAL REF. & TEST	SPECIFICATION	Test RESULT	UNITS
Internal control recover (Reference standard 4.2 ng/ml)	80 – 120	114 4.8	% ng/mL
Sensitivity (Ligand detection limit)	≤ 1	Conform	ng/mL
Calibration curve (ELISA)	Conform	See below	
TMB incubation time (Thermo 1-Step Ultra TMB-ELISA)	2-20	10	minutes

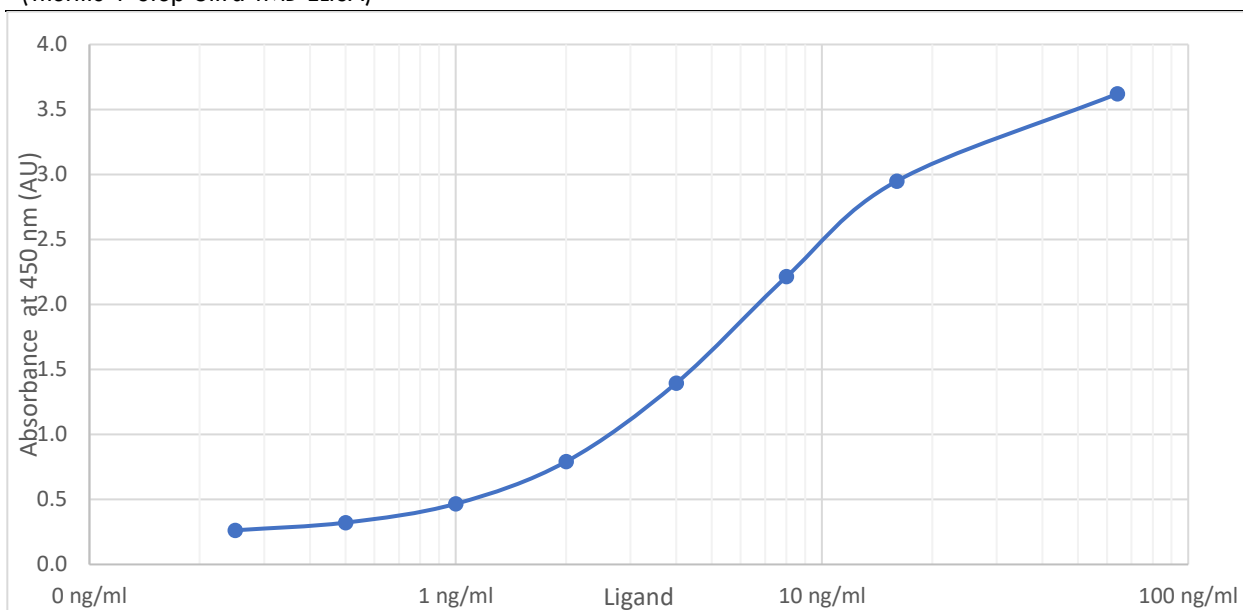

Example of calibration curve, Lot 101017-211 (y-axis OD_{450nm}; x-axis [Ligand] in ng/mL)
FOR RESEARCH ONLY. NOT INTENDED FOR HUMAN USE

Product management

Date: 28-Jun-2022