

Test Report

– Eppendorf PCR clean & sterile –

1 Set epT.I.P.S.[®] Motion Reloads

**1 - 50 μ L, 2304 pcs.
Eppendorf Filtertips
PCR clean / sterile**




Read the instruction for use on
www.eppendorf.com/manuals



2030-06

LOT 0222053L

STERILE R

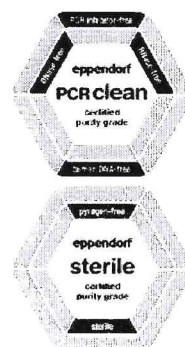

Eppendorf SE
22331 Hamburg · Germany
Tel: +49 1 803 666 789
E-Mail: eppendorf@eppendorf.com

Order no.: 0030 014.529

Distributed in North America by
Eppendorf North America · USA
Tel: +1 800 645 3050
E-Mail: info@eppendorf.com

Cat. no.: 0030014529

Made in Germany

eppendorf

• **Human DNA**

Method: *real-time* PCR acc. to SOP 99880/V8
Limit: < 2 pg; less than one human cell

• **DNase**

Method: DNA Digestion acc. to SOP 100570/V4
Limit: Not detectable
(LOD: 1.0×10^{-7} Kunitz units)

• **RNase**

Method: RNA Digestion acc. to SOP 100571/V4
Limit: Not detectable
(LOD: 1.0×10^{-9} Kunitz units)

• **PCR Inhibition**

Method: *real-time* PCR acc. to SOP 100559/V4
Limit: less than 10 targets amplifiable

• **Sterility**

Method: Sterilization with SAL 10^{-6} by
R: Irradiation according DIN EN ISO 11137
Test method: USP, Ph. Eur. 10.0 / 2.6.12

• **Endotoxin**

Method: Kinetic-chromogenic LAL test (Ph. Eur. 10.0 / 2.6.14)
Limit: < 0.001 EU/mL

Customer: Eppendorf SE, Barkhausenweg 1, D-22339 Hamburg

Date of sample receipt / examination: 24.07.25

Testing of the rinse solution of the above described lot showed conformity within the limits of detection.

30.07.25

Date of release

Epp 2507-6127

Registration number

i.v. T. C. K.

Dr. rer. nat. Sybille Kuhnert (Head)

The test results refer exclusively to the items tested as arrived. The test report must not be copied partially without the approval of LADR GmbH.

page 1 of 1