

TaqPath™ 1-Step Multiplex Master Mix

Product No: A28525 A28526 A28527
 Quantity: 1 x 0.5 mL 5 x 1 mL 1 x 10 mL
 Packaging Lot¹: 2815429
 Expiration Date: 31 January 2025
 Storage: -30 to -10°C
 Bulk Lot²: 2775521

Manufactured according to current good manufacturing practices (cGMP) and subjected to a panel of quality control tests to ensure the highest level of performance and lot-to-lot consistency.

Analytical Methods

| Parameter | QC method | Specification | Result |
|---|---|--|----------|
| Magnesium ion (Mg ²⁺) concentration | High performance ion chromatography with the detection of conductivity signal is performed on the product and standards. | 24.48 – 33.12 mM | Conforms |
| Potassium ion (K ⁺) concentration | | 170 – 230 mM | Conforms |
| DNase Level | DNase levels are measured using a modified DNA oligonucleotide possessing a quencher and fluorescent label that emits a fluorescent signal when cleaved by DNase. | Samples have ≤ 44.0 pg / 5 µL | Conforms |
| E.coli DNA Level | E. coli DNA levels are quantified via qPCR utilizing a standard curve with four replicates for each point. | ≤ 10 copies of E. coli DNA / 50 µL Reaction Volume | Conforms |
| pH | The pH value is measured at a temperature of 25 °C. | 7.95 – 8.25 | Conforms |

Note: Enzyme bulk is tested for activity and E.coli DNA Level


Functional Tests

TaqPath™ 1-Step Multiplex Master Mix is tested for performance using a panel of two quadplex assay combinations and 4 simplex Gene Expressions assays. The first quadplex assay combination consists of 4 Gene Expression assays run with a serial dilution of human RNA. The second quadplex assay combination consists of three Gene Expression assays coupled with an exogenous internal positive control (IPC) reagent. The second quadplex and four simplex reactions are run at one concentration of purified human RNA. Performance attributes evaluated include PCR efficiency, R2 value, Ct Value, and Absolute Delta Ct between Quadplex and Simplex.

| Quadplex 1 | PCR Efficiency | R ² Value | Result |
|---------------------|----------------|----------------------|----------|
| Assay Hs00164924_m1 | 85% - 115% | ≥ 0.95 | Conforms |
| Assay Hs99999909_m1 | 85% - 115% | ≥ 0.95 | Conforms |
| Assay RNaseP | 85% - 115% | ≥ 0.95 | Conforms |
| Assays GAPDH | 85% - 115% | ≥ 0.95 | Conforms |

| Quadplex 2 | Average Ct Value | Ct Std. Dev. | Result |
|--------------------------------------|------------------|--------------|----------|
| Assay Exogenous IPC (quadplex assay) | 27.18 – 31.48 | ≤ 0.4 | Conforms |

| Simplex | Absolute Delta Ct (Simplex vs Multiplex) | Result |
|---------------------|--|----------|
| Assay Hs00164924_m1 | < 1.5 | Conforms |
| Assay Hs99999909_m1 | < 1.5 | Conforms |
| Assay RNaseP | < 1.5 | Conforms |
| Assays GAPDH | < 1.5 | Conforms |

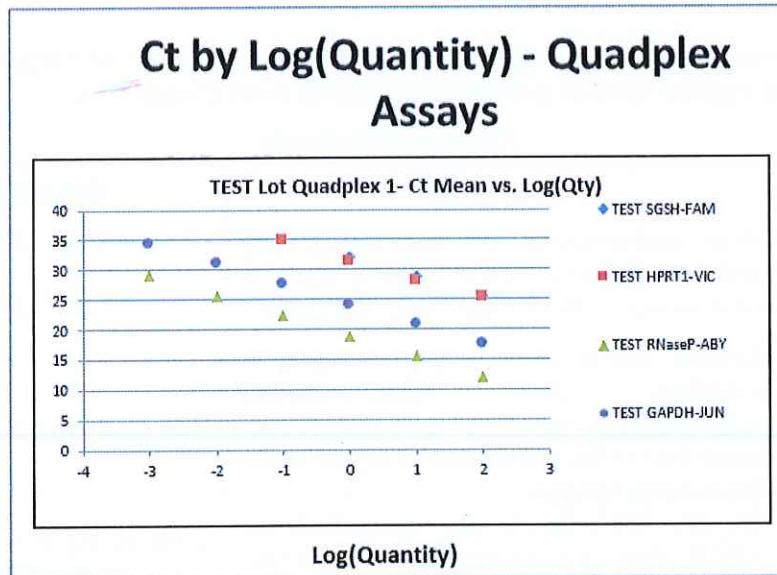

Quality Signature: Audronė Lakštauskienė

Date: 29 September 2023

For Laboratory Use

¹ Packaging Lot is the unique Lot # assigned to the packing event of the vials into the product boxes.

² Bulk Lot is the unique Lot # assigned to the production Lot prior to filling. Note: It is possible for different packing Lot's to be filled by the same bulk Lot.